

# Phototherapy Device Instructions



## USAGE INSTRUCTIONS

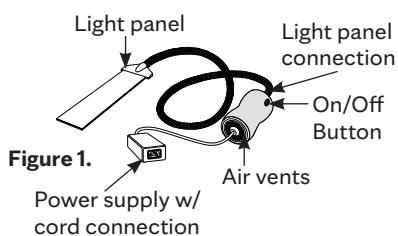


Figure 1.

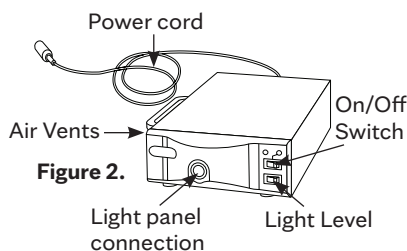


Figure 2.

- 1 Find a hard-flat surface on which to place the device. Ensure air vents on device are not blocked. (Figure 1. - BiliTx Model) (Figure 2. - Wallaby 3 Model)




Figure 3.

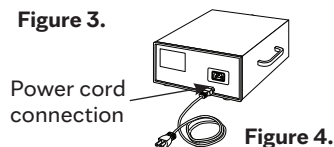


Figure 4.

- 2 Plug device into a grounded wall outlet. (Figure 3. - BiliTx Model) (Figure 4. - Wallaby 3 Model)

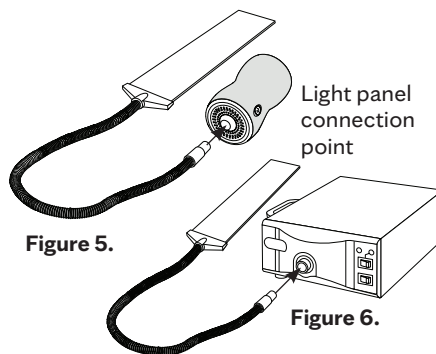


Figure 5.

- 3 Place the metal collar of the panel into the device. (Figure 5. - BiliTx Model) (Figure 6. - Wallaby 3 Model)

- 4 Turn on the device and ensure that light side of panel is facing up.

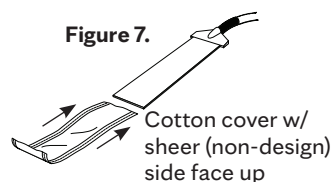


Figure 7.

- 5 Place panel into cotton cover ensuring that the light side faces the sheer side of the cover (should be the non-design side of the cotton cover). (Figure 7.)




Figure 8.

- 6 Place the now covered panel under the baby and around the torso ensuring that the sheer side of the cover is touching the baby's skin. (Figure 8.)

- 7 Leave the device on the baby as long as possible.
- 8 When providing treatment, you may cuddle, feed, or pick up your baby at any time during the therapy. (Stay close to the device to avoid pulling the device off its placed surface)
- 9 Upon completion of treatment turn off device and unplug from outlet.
- 10 Let the device cool down for 15 minutes before moving to another area.

## CLEANING INSTRUCTIONS

### As needed:

- 1 Wipe panel with damp cloth allowing to full air dry before next use. **Never** attempt to wash the panel either by submersion, dish washer, or washing machine.
- 2 Dispose of and replace cotton covers if soiled.

## MAINTENANCE INSTRUCTIONS

### Weekly:

- 1 Mayo Clinic Store provided phototherapy devices should only be maintained by a Mayo Clinic Store employee who is a trained technician. Patients should avoid any disassembly of the phototherapy device or its accessories.

DEVICE TROUBLESHOOTING

\*Patients should avoid any disassembly of the phototherapy device. If unable to effectively troubleshoot the device patients should contact the Mayo Clinic Store for further assistance.

ISSUE	CHECK
Device has no power	<ul style="list-style-type: none"><li>• Verify that device power cord is firmly plugged into the electrical outlet and not in an outlet controlled by a wall switch.</li><li>• Verify the power cord to the device is still connected.</li><li>• Check the power cord for rips or tears.</li></ul>
Device panel is not illuminating	<ul style="list-style-type: none"><li>• Verify the panel's metal collar is properly locked/connected to the main device.</li></ul>

DEVICE RENTAL PERIOD

This device is a **daily rental**. Return promptly once the physician discontinues therapy to avoid continued billing charges.

SAFE USE INSTRUCTIONS

- Always place device on a hard, flat surface outside the crib. Never place device in or on a crib.
  - Do not use device while bathing baby.
  - Do not place or store the device where it can fall or be pulled into a tub or sink.
  - Do not leave device on when not being used for treatment.
- Always turn off and unplug the device when cleaning the panel.
  - Do not use device near combustible or flammable materials.
  - Do not use near an individual that is using or being administered oxygen.
  - Do not use extension cords or power strips to power the device.
- Never operate the device if it has a damaged cord or plug.
  - Do not block the air vents on the device, this would cause it to overheat.

SERVICE LOCATIONS

The Mayo Clinic Store is available to assist with questions related to your phototherapy device. Normal business hours for the Mayo Clinic Stores is Monday through Friday, 8 am–5 pm. For issues that cannot wait until the next business day contact the store where you received your equipment for further assistance.

MINNESOTA	WISCONSIN
<b>Mankato</b>	<b>La Crosse</b>
Call 507-594-2689	Call 608-392-9797
	<b>Onalaska</b>
	Call 608-392-9797